

## ALCOTEST 9510 PARAMETER REPORT

### Equipment

Serial No.: ARMK-0265  
Firmware: 8326739 1.5  
WinCE application: 8326738 2.9  
Configuration: 8326737 3.10

Date: 01/08/2025  
Time: 09:47:20

### Parameter

min. blow time	5.0	s
min. breath volume for females of age 60+	1.2	L
min. breath volume for all other	1.5	L
min. blow flow	4.5	L/min
plateau detection limit	4	%
plateau detection start conc.	70	microgram/L
neg. flow detection (part. vacuum)	10.0	hPa
neg. flow detection sensitivity	10	
cal. gas abort volume	0.4	L
result-to-zero limit	0.0050	%BAC
ambient air check limit	0.0049	%BAC
interference det. d-criterion limit abs.	38	microgram/L
interference det. d-criterion limit rel.	10.0	%
interference det. t-criterion limit abs.	8	microgram/L
interference det. t-criterion limit rel.	2.1	%
IR CO2 offset	10	microgram/L
IR H2O offset	4	microgram/L
EC H2O offset	0	microgram/L
Value-based EC aging comp. on/off (1/0)	0	
Time-based EC aging comp. on/off (1/0)	1	
Time-based EC aging comp. per month	0.2	%
Time-based EC aging comp. maximum	3.0	%
EC fatigue comp. max. sum	15000	
EC fatigue comp. factor	50	
EC fatigue comp. minutes	180	
mouth alc. mark limit	500	
mouth alc. lower limit	30	
mouth alc. slope	6	
mouth alc. zero limit	50	
mouth alc. max. neg. sum	6	
mouth alc. max. 2nd derivative	35	

**ALCOTEST 9510 CERTIFICATION REPORT - WET ADJUST (PART I)**  
*Seaside Heights*

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMK-0265  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Wet Adjust Record**

Wet Adjust File No.: 144 Wet Adjust Date: 01/08/2025 Wet Adjust No.: 4  
Wet Adjust Time: 10:39:13  
Concentration: 0.100 %  
Adjusting Unit: X-Cal 2000 Adj. Unit Ser. No.: ARMN-0039 Adj. Unit Exp.: 10/04/2025  
Solution Lot No.: 23240 Soln. Bottle No.: 833 Adjust Soln. Exp.: 06/28/2025  
Preadjust Simulator Temp.: 34.00 degree C  
Postadjust Simulator Temp.: 34.00 degree C

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: Bellay - First Name: David MI: M. Badge No.: 8112

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.



Signed:

Date: 01/08/2025

ID: 50

**ALCOTEST 9510 CERTIFICATION REPORT - DRY ADJUST (PART II)**  
*Seaside Heights*

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMK-0265  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Dry Adjust Record**

Dry Adjust File No.: 145 Dry Adjust Date: 01/08/2025 Dry Adjust No.: 4  
Dry Adjust Time: 11:06:55

Concentration: 0.100 %  
Dry Gas Lot No.: 302-402448282 Adjust Gas Exp.: 05/20/2025  
Barom. Model No.: Mensor CPG2300 Barom. Serial No.: 41001RDH Barom. Cert. Exp.: 09/26/2025  
Pre-adjust Amb. Pressure: 1015 hPa Post-adjust Amb. Pressure: 1015 hPa

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: Bellay - First Name: David MI: M. Badge No.: 8112

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.



Signed:

Date: 01/08/2025

ID: 50

**ALCOTEST 9510 CERTIFICATION REPORT - LINEARITY (PART III)**  
*Seaside Heights*

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMK-0265  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Linearity Record**

Linearity File No.: 146 Lin. Date: 01/08/2025 Lin. No.: 4

0.040% Dry Gas Lot No.: 302-402755169 Adjust. Gas Exp.: 05/25/2026  
0.080% Dry Gas Lot No.: 302-402477284 Adjust. Gas Exp.: 06/27/2025  
0.160% Dry Gas Lot No.: 302-402486005 Adjust. Gas Exp.: 07/13/2025  
0.300% Dry Gas Lot No.: 302-402759888 Adjust. Gas Exp.: 05/31/2026

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	11:27:44		*TEST PASSED*
Control .04 Test 1 EC	0.038	11:28:19	1015	*TEST PASSED*
Control .04 Test 1 IR	0.039	11:28:19	1015	*TEST PASSED*
Ambient Air Blank	0.000	11:29:25		*TEST PASSED*
Control .04 Test 2 EC	0.039	11:29:36	1015	*TEST PASSED*
Control .04 Test 2 IR	0.039	11:29:36	1015	*TEST PASSED*
Ambient Air Blank	0.000	11:31:06		*TEST PASSED*
Control .08 Test 3 EC	0.078	11:31:40	1015	*TEST PASSED*
Control .08 Test 3 IR	0.079	11:31:40	1015	*TEST PASSED*
Ambient Air Blank	0.000	11:32:54		*TEST PASSED*
Control .08 Test 4 EC	0.080	11:33:06	1015	*TEST PASSED*
Control .08 Test 4 IR	0.080	11:33:06	1015	*TEST PASSED*
Ambient Air Blank	0.000	11:35:15		*TEST PASSED*
Control .16 Test 5 EC	0.154	11:35:49	1015	*TEST PASSED*
Control .16 Test 5 IR	0.157	11:35:49	1015	*TEST PASSED*
Ambient Air Blank	0.000	11:37:10		*TEST PASSED*
Control .16 Test 6 EC	0.158	11:37:23	1015	*TEST PASSED*
Control .16 Test 6 IR	0.158	11:37:23	1015	*TEST PASSED*
Ambient Air Blank	0.000	11:44:15		*TEST PASSED*
Control .30 Test 7 EC	0.297	11:44:51	1014	*TEST PASSED*
Control .30 Test 7 IR	0.302	11:44:51	1014	*TEST PASSED*
Ambient Air Blank	0.000	11:46:19		*TEST PASSED*
Control .30 Test 8 EC	0.303	11:46:32	1014	*TEST PASSED*
Control .30 Test 8 IR	0.305	11:46:32	1014	*TEST PASSED*
Ambient Air Blank	0.000	11:47:08		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Bellay - First Name: David MI: M. Badge No.: 8112

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.



Signed:

Date: 01/08/2025

ID: 50

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 1**  
*Seaside Heights*  
**SERIAL NUMBER: ARMK-0265**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMK-0265  
 Firmware: 8326738 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9  
 Cyl1 Install File No.: 111 Cyl1 Install Date: 07/29/2024 Cyl1 Install No.: 2

**Control Tests (0.100%)**

Installation Inlet: #1 (Upper) Post test active Cyl.: #2 (Lower)  
 Dry Gas Lot No.: 302-402843438 Dry Gas Lot Exp.: 09/08/2026

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	10:17:45		*TEST PASSED*
Control Test 1			1016	*TEST PASSED*
EC Result	0.097	10:18:31		*TEST PASSED*
IR Result	0.100	10:18:31		*TEST PASSED*
Ambient Air Blank	0.000	10:19:43		*TEST PASSED*
Control Test 2			1016	*TEST PASSED*
EC Result	0.100	10:20:07		*TEST PASSED*
IR Result	0.100	10:20:07		*TEST PASSED*
Ambient Air Blank	0.000	10:21:21		*TEST PASSED*
Control Test 3			1016	*TEST PASSED*
EC Result	0.100	10:21:45		*TEST PASSED*
IR Result	0.100	10:21:45		*TEST PASSED*
Ambient Air Blank	0.000	10:22:17		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Waldrop - First Name: Robert MI: W Badge No.: 8256

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*TH Waldrop # 8256*

Signed:

Date: 07/29/2024

ID: 52

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 2**  
*Seaside Heights*  
**SERIAL NUMBER: ARMK-0265**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMK-0265  
 Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9  
 Cyl2 Install File No.: 27 Cyl2 Install Date: 12/04/2023 Cyl2 Install No.: 1

**Control Tests (0.100%)**

Installation Inlet: #2 (Lower) Post test active Cyl.: #1 (Upper)  
 Dry Gas Lot No.: 302-402755079 Dry Gas Lot Exp.: 05/31/2026

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	09:55:21		*TEST PASSED*
Control Test 1			1010	*TEST PASSED*
EC Result	0.099	09:56:07		*TEST PASSED*
IR Result	0.100	09:56:07		*TEST PASSED*
Ambient Air Blank	0.000	09:57:11		*TEST PASSED*
Control Test 2			1010	*TEST PASSED*
EC Result	0.100	09:57:35		*TEST PASSED*
IR Result	0.100	09:57:35		*TEST PASSED*
Ambient Air Blank	0.000	09:58:39		*TEST PASSED*
Control Test 3			1010	*TEST PASSED*
EC Result	0.101	09:59:03		*TEST PASSED*
IR Result	0.101	09:59:03		*TEST PASSED*
Ambient Air Blank	0.000	09:59:26		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Lutz - First Name: Dennis MI: J Badge No.: 7045

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*J. P. Lutz 7045*

Signed:

Date: 12/04/2023

ID: 5

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401036

**DRAEGER MEDICAL SYSTEMS INC**

Sales order: 1123816776

Date: September 18, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer

ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.

CALGAZ LOT#: 302-402843436

ETHANOL IN NITROGEN

Product Expiration: September 08, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	263.3	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398873.

#### Analytical:

Analytical instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: September 08, 2023

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400

Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

**DRAEGER MEDICAL SYSTEMS INC.;**

Sales order: 1121656187  
Date: June 30, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY:  $\pm 0.002$  BrAC or  $\pm 2\%$  whichever is greater.  
CALGAZ LOT#: 302-402755079  
ETHANOL IN NITROGEN

Product Expiration: May 31, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	262.5	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3446312 and 3398673.

**Analytical:**

Analytical Instruments Calibrated Using NMI Traceable Standards.


Certification Numbers: A679-20190918; D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 31, 2023

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251





# Dräger

## Alcotest 9510

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 9510 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest 9510 is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

10/31/2023

ARMK-0265

Draeger, Inc.

BLS IP



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

TAHESHA L. WAY
Lt. Governor

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 09/13/2023

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 23240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1196 to 0.1212 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 28, 2025.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Signature of Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15 day of September, 2023.

Signature of Notary Karen E. Stahl

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



**Customer:** DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
**PO Number:** S1O4303440829

**Certificate/SO Number:** 5-F2R00-120-1 Revision 0

**Manufacturer:** Drager Safety AG & Co. KGaA  
**Model Number:** X-Cal 2000  
**Description:** Breath Alcohol Simulator  
**Serial Number:** ARMN-0039  
**ID:** NONE

**As-Found:** In Tolerance  
**As-Left:** In Tolerance

**Issue Date:** Oct 04, 2024  
**Calibration Date:** Oct 04, 2024  
**Due Date:** Oct 04, 2025

**Calibrated To:** Customer Spec  
**Calibration Procedure:** 1-AC103519-1

Transcat Calibration Laboratories have been audited and found in compliance with ISO/IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Transcat Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not certify or cover an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements, ISO 9001:2015 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS16949:2009, 10CFR21, 10CFR50 App. B, ASME NQA-1:2012, and ANSI/NCSL Z540.3-2010 are covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national metrology institutes (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type methods. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination.

Uncertainties are reported with a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations). The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-18. For mass calibrations: Conventional mass referenced to 8.0 g/cm<sup>3</sup>.

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The date of the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturers (OEM's) warranted specifications or specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).

**Date Received:** October 01, 2024  
**Service Level:** R9

**Certificate - Page 1 of 5**  
Reprinted on October 18, 2024

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085

PO Number: S104303440829

Certificate/SO Number: 5-F2R00-120-1 Revision 0

**As Found/As Left Data**

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found / As Left	O O T	Cal Proces Uncertain (k=2; ±)
<b>Function Checks</b>							
Bubble Check			P	P	P		
Seal Check			P	P	P		
<b>Temperature Source: Accuracy Test</b>							
Accuracy Test	34.00°C	±(0.02 °C)	33.98	34.02	34.00 °C		1.5e-002
<b>Temperature Source: Stability Test</b>							
Stability Test	0.00°C	±(0.02 °C)	-0.02	0.02	0.00 °C		5.0e-003

**Traceable Standards**

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date
05H1431	AccuMac Corporation	AM1760	Secondary SPRT	12-Feb-24	28-Feb-25
HP927312	Hart Scientific/Fluke	1575	Super Thermometer	10-Jul-24	31-Jan-26

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.

**Environmental Data**

Temperature	Relative Humidity	Temp / RH Asset	Lab Area
70.60°F /21.44°C	53.90%	DewK5	G

**Decision Rule**

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measu

Date Received: October 01, 2024  
Service Level : R9

Certificate - Page 2 of 5

Reprinted on October 18, 2024

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085

PO Number: S104303440829

---

**Certificate/SO Number: 5-F2R00-120-1 Revision 0**

---

are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone is identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op Fail R document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. States

Date Received: October 01, 2024  
Service Level: R9

**Certificate - Page 3 of 5**  
Reprinted on October 18, 2024

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085

PO Number: S104303440829

Certificate/SO Number: 5-F2R00-120-1 Revision 0

**Legend**

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold the
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (k)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OOA	Out of Acceptance (#)
OOT	Out of Tolerance (*)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

Date Received: October 01, 2024  
Service Level : R9

Certificate - Page 4 of 5

Reprinted on October 18, 2024

**Customer:** DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085


**PO Number:** S104303440829

**Certificate/SO Number:** 5-F2R00-120-1 Revision 0

---

**Calibrated At:**  
16115 Park Row  
Houston, TX 77084

**Facility Responsible:**  
16115 Park Row  
Houston, TX 77084  
800-828-1470

**Calibrated By:**  
 **Electronically Signed By:**  
Jose Martinez

**Unit Barcode:**



0900B587243

**Date Received:** October 01, 2024  
**Service Level :** R9

---

Jose Martinez                      Oct 04, 2024  
Calibration Technician              02:35:04 -04:00

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S1O4303405716

Certificate/SO Number: 5-F2D8A-40-1 Revision 0

Manufacturer: Wika Instr/Mensor Corp/Trend  
Model Number: CPG2300  
Description: Portable Barometer  
Serial Number: 41001RDH  
ID: NONE

As-Found: In Tolerance  
As-Left: In Tolerance

Issue Date: Sep 27, 2024  
Calibration Date: Sep 26, 2024  
Due Date: Sep 26, 2025

Calibrated To: Manufacturer S  
Calibration Procedure: 1-AC94879-0

Transcat Calibration Laboratories have been audited and found in compliance with ISO/IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the present Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not cover an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements, Z540.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS16949:2009, 10CFR21, 10CFR50 App. B, ASME NQA-1:2012, and ANSI/NCSL Z540.3-covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type methods. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination.

Uncertainties are reported with a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass) unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-18. For mass calibrations: Conventional mass referenced to 8.0 g/cm<sup>3</sup>.

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The date of the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturers (OEM's) warranted specification tolerances. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).

Date Received: September 03, 2024  
Service Level: R9

Certificate - Page 1 of 5  
Reprinted on October 17, 2024



Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085

PO Number: S104303405716

Certificate/SO Number: 5-F2D8A-40-1 Revision 0

As Found/As Left Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found / As Left	O O T	Cal Proces Uncertaint (k=2; ±)
Pressure Measure: 8 to 17 psia Range							
	7.985psia	±(0.015% FS)	7.982	7.988	7.985 psia		1.5e-004
	8.857psia	±(0.015% FS)	8.854	8.860	8.856 psia		1.7e-004
	9.731psia	±(0.015% FS)	9.728	9.734	9.731 psia		1.8e-004
	10.628psia	±(0.015% FS)	10.625	10.631	10.627 psia		2.0e-004
	11.647psia	±(0.015% FS)	11.644	11.650	11.647 psia		2.2e-004
	12.523psia	±(0.015% FS)	12.520	12.526	12.523 psia		2.4e-004
	13.396psia	±(0.015% FS)	13.393	13.399	13.395 psia		2.5e-004
	14.269psia	±(0.015% FS)	14.266	14.272	14.269 psia		2.7e-004
	15.270psia	±(0.015% FS)	15.267	15.273	15.269 psia		2.9e-004
	16.145psia	±(0.015% FS)	16.142	16.148	16.145 psia		3.1e-004
	17.020psia	±(0.015% FS)	17.017	17.023	17.019 psia		3.2e-004
	13.396psia	±(0.015% FS)	13.393	13.399	13.395 psia		2.5e-004
	12.523psia	±(0.015% FS)	12.520	12.526	12.523 psia		2.4e-004
	11.647psia	±(0.015% FS)	11.644	11.650	11.647 psia		2.2e-004

Date Received: September 03, 2024  
Service Level: R9

Certificate - Page 2 of 5

Reprinted on October 17, 2024

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085

PO Number: S104303405716

Certificate/SO Number: 5-F2D8A-40-1 Revision 0

**Traceable Standards**

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date
DW09BA	Fluke/DH Instruments	PG7601	Piston Gauge	11-Sep-23	30-Sep-24
DW09CA	DH Instruments	MS-AMH-38	AMH Mass Set	13-Sep-24	13-Dec-24
DW09LOW	Fluke/DH Instruments	PC-7100/7600-10-TC	Gas Piston-Cylinder Module	22-Aug-23	31-Aug-28
DW09MASS	Fluke/DH Instruments	MS-AMH-38	AMH Mass Set	1-Feb-24	30-Nov-24

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.

**Environmental Data**

Temperature	Relative Humidity	Temp / RH Asset	Lab Area
71.20°F /21.78°C	42.50%	DewK8	B

**Decision Rule**

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurements are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the rejection zone, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone is identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op Fail R document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. State

Date Received: September 03, 2024  
Service Level : R9

Certificate - Page 3 of 5

Reprinted on October 17, 2024

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085

PO Number: S104303405716

Certificate/SO Number: 5-F2D8A-40-1 Revision 0

**Legend**

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold the
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (k)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OOA	Out of Acceptance (#)
OOT	Out of Tolerance (*)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

Date Received: September 03, 2024  
Service Level: R9

Certificate - Page 4 of 5

Reprinted on October 17, 2024

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085


PO Number: S1O4303405716

Certificate/SO Number: 5-F2D8A-40-1 Revision 0

---

Calibrated At:  
16115 Park Row  
Houston, TX 77084

Facility Responsible:  
16115 Park Row  
Houston, TX 77084  
800-828-1470

Calibrated By:  
 Electronically Signed By:  
Alex Spilker

---

Alex Spilker                      Sep 26, 2024  
Calibration Technician        21:33:01 -04:00

Unit Barcode:   
0900B581608

Date Received: September 03, 2024  
Service Level : R9

**Certificate - Page 5 of 5**  
Reprinted on October 17, 2024

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

NJSP DEPT OF LAW AND PUBLIC SAFETY

Sales order: 1111663404  
Date: July 05, 2022

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402448282  
ETHANOL IN NITROGEN

Product Expiration: May 20, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	263.3	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283190, 283189, 283188, or 283192 dated 6th January 2022 applies

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 20, 2022

APPROVED BY: \_\_\_\_\_

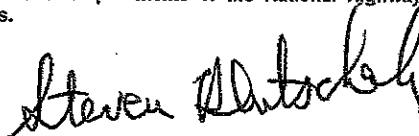

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

DRAEGER MEDICAL SYSTEMS INC.;

Sales order: 1121156486

Date: June 12, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer

ANALYTICAL ACCURACY:  $\pm 0.002$  BrAC or  $\pm 2\%$  whichever is greater.

CALGAZ LOT#: 302-402755169

ETHANOL IN NITROGEN

Product Expiration: May 25, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	104.2PPM	(0.040)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	107.2	(0.041)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 25, 2023

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400

Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

**DRAEGER MEDICAL SYSTEMS INC.;**

Sales order: 1113360565

Date: August 29, 2022

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer

ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.

CALGAZ LOT#: 302-402477284

ETHANOL IN NITROGEN

Product Expiration: June 27, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	208.4PPM	(0.080)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	210.9	(0.081)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283192, dated 6th January 2022 or calibration test 292029, 292030 or 292031, dated 26th March 2022 applies

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: June 27, 2022

APPROVED BY: \_\_\_\_\_

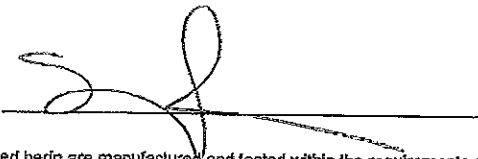

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400

Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

NJSP

Sales order: 1111788955

Date: July 14, 2022

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer

ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.

CALGAZ LOT#: 302-402486005

ETHANOL IN NITROGEN

Product Expiration: July 13, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	416.8PPM	(0.160)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	420.0	(0.161)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283192, dated 6th January 2022 or calibration test 292029, 292030 or 292031, dated 26th March 2022 applies

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: July 13, 2022

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400

Fax: (410) 228-4251



# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401041NJ  
DRAEGER MEDICAL SYSTEMS INC

Sales order: 1123022087  
Date: August 18, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402759888  
ETHANOL IN NITROGEN

Product Expiration: May 31, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	781.5PPM	(0.300)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	793.1	(0.304)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 31, 2023

APPROVED BY:

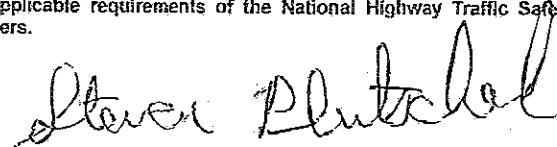

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request"

CALGAZ, a division of Airgas USA LLC  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**David M. Bellay**

**New Jersey State Police**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 28th DAY OF April

TWO THOUSAND AND Twenty Three

*[Signature]*  
COLONEL  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 10/22)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**David M. Bellay**

**Breath Test Coordinator/Instructor**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 20th DAY OF August

TWO THOUSAND AND Twenty Four

*[Signature]*  
COLONEL  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 10/22)

DEPARTMENT OF  
*Law and Public Safety*  
 This is to certify that

Robert W. Waldrop

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 25th DAY OF March

TWO THOUSAND AND Twenty Four

*[Signature]*  
 COLONEL  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 10/22)

DEPARTMENT OF  
*Law and Public Safety*  
 This is to certify that

Robert W. Waldrop

New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 28th DAY OF April

TWO THOUSAND AND Twenty Three

*[Signature]*  
 COLONEL  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 10/22)

DEPARTMENT OF  
**Data and Public Safety**  
*This is to certify that*

**Dennis J. Lutz**

**New Jersey State Police**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION,  
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 8th DAY OF June

TWO THOUSAND AND Twenty One

*[Signature]*  
 COLONEL  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	7/13/23	Hamilton Tech	R. G.
2.			
3.			
4.			
5.			
6.			
7.			
8.			
9.			

S.P. 293B (Rev. 01/18)

DEPARTMENT OF  
**Data and Public Safety**  
*This is to certify that*

**Dennis J. Lutz**

**Breath Test Coordinator/Instructor**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION,  
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 8th DAY OF June

TWO THOUSAND AND Twenty One

*[Signature]*  
 COLONEL  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

	DATE	Refresher Course PLACE	INSTRUCTOR
1.			
2.			
3.			
4.			
5.			
6.			
7.			
8.			
9.			

S.P. 293B (Rev. 01/18)